



ANALIZA BIAŁEK



100016160

Laboratory of Analysis

Client: AVENOR
Order number: 100016160
Name: AVENOR BPC-157+TB-500
Number of samples: 1 vial

Batch number: -----
Receive date: 2026-07-13
Start date: 2026-07-22
End date: 2026-07-24

Sample identification

Substance	Method of taking a sample	Form
BPC-157, TB-500	Sample provided by customer	White powder in glass vial


Results

Substance	Sample name	Content	Purity
BPC-157	AVENOR BPC-157+TB-500 10MG+10MG	10,34mg	99%
TB-500	AVENOR BPC-157+TB-500 10MG+10MG	10,98mg	99%

Research comment

The test sample was applied in the amount of 3µl to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H₂O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peaks of the sought substances appeared. Its concentration, when compared to the reference chromatogram shows the table above. Height the measurement error is + - 0,05 mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample

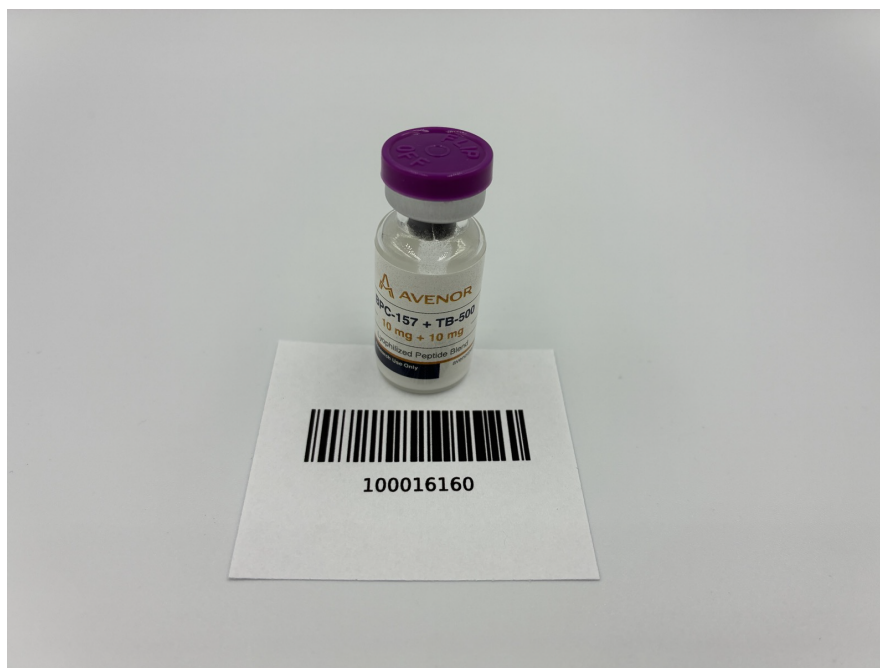

Password

D3M18U7A

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac




ANALIZA BIAŁEK



100016160

Chromatogram

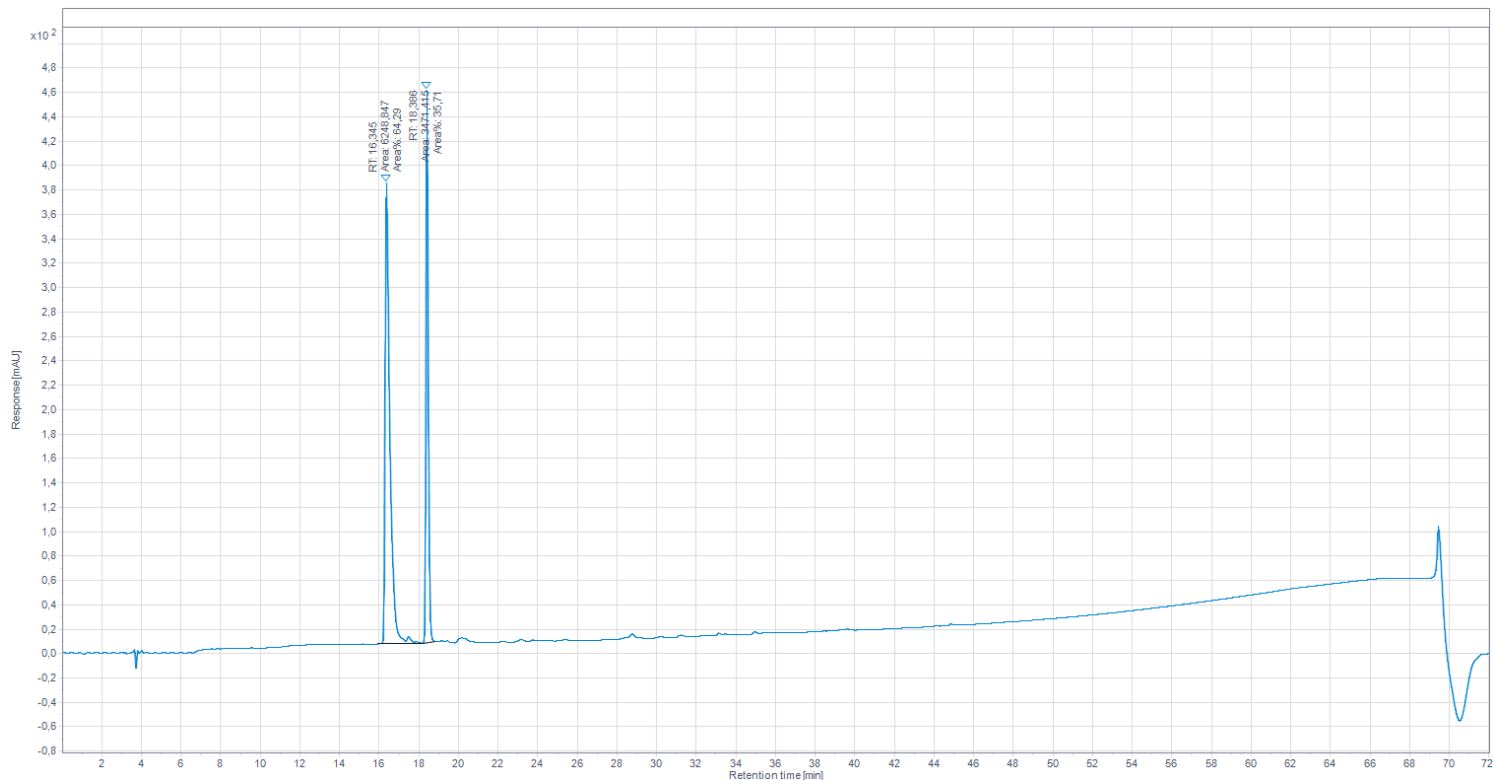

Method

Time	H2O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
60min	5%	95%
62min	5%	95%

Password

D3M18U7A

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:

Analysis and research specialist
mgr Arkadiusz Zajac